



TOMOWELL GLOVES





NITRILE GLOVES



PRODUCT SPECIFICATIONS

<i>Material</i>	<i>Nitrile</i>
<i>Type</i>	<i>Non-Sterile Powder-Free</i> <i>Ambidextrous; Finger Tip Texture; Beaded Cuff; Blue and White</i>
<i>Quality Standards</i>	<i>Manufactured under ISO 9001:2015, ISQ, ISO 13485:2016, FDA, CE</i> <i>Quality Management System.</i> <i>Manufactured from 100% nitrile (Acrylonitrile-Butadiene)</i>
<i>Gloves Size</i>	<i>Extra Small, Small, Medium, Large, Extra Large</i> <i>Black marked in the check box on the shipping carton</i>
<i>Storage</i>	<i>Store in a cool and dry place, temperature is not higher than 38°C</i>
<i>Shelf-life</i>	<i>3 years from the date of manufacturing.</i>

PHYSICAL PROPERTIES AND BIOCOMPATIBILITY

Tensile	Tensile strength (MPA) <i>(Before Aging)</i> : 18Mpa min <i>(After Aging)</i> : 20Mpa Min	Tensile strength (MPA) <i>(Before Aging)</i> : 14Mpa min <i>(After Aging)</i> : 14Mpa Min
	Elongation at break (%) <i>(Before Aging)</i> : 600% min <i>(After Aging)</i> : 500% min	Elongation at break (%) <i>(Before Aging)</i> : 500% min <i>(After Aging)</i> : 400% min
<i>Powder Content</i>	<i>2 mg/glove maximum</i>	
<i>Protein Content</i>	<i>Protein Free</i>	


Functional Benefits

- Protection from unwanted and dangerous substances
- Beaded cuff ensures easy donning and prevent roll down
- Superior strength with better puncture resistance
- Full textured or Finger Tip textured enhances wet and dry grip
- Thinner gauge improves tactile sensitivity
- Custom design enhances comfort and fit
- Provide an alternative solution for individuals who are allergic to natural rubber latex

PHYSICAL DIMENSIONS


DIMENSIONS	Standards	
	MEDB GLOVE	ASTM D6319
(mm) <i>Length</i>	230 min	220 min (XS,S) 230 min (M,L,XL)
(mm) <i>Width</i>	75 ± 5 (XS) 85 ± 5 (S) 95 ± 5 (M) 105 ± 5 (L) 115 ± 5 (XL)	70 ± 10 (XS) 80 ± 10 (S) 95 ± 10 (M) 110 ± 10 (L) 120 ± 10 (XL)
(mm) <i>Thickness-Single wall</i>	(Fingers): 0.08 mm min (Palm): 0.06 mm min	(Fingers): 0.05 mm min (Palm): 0.05 mm min



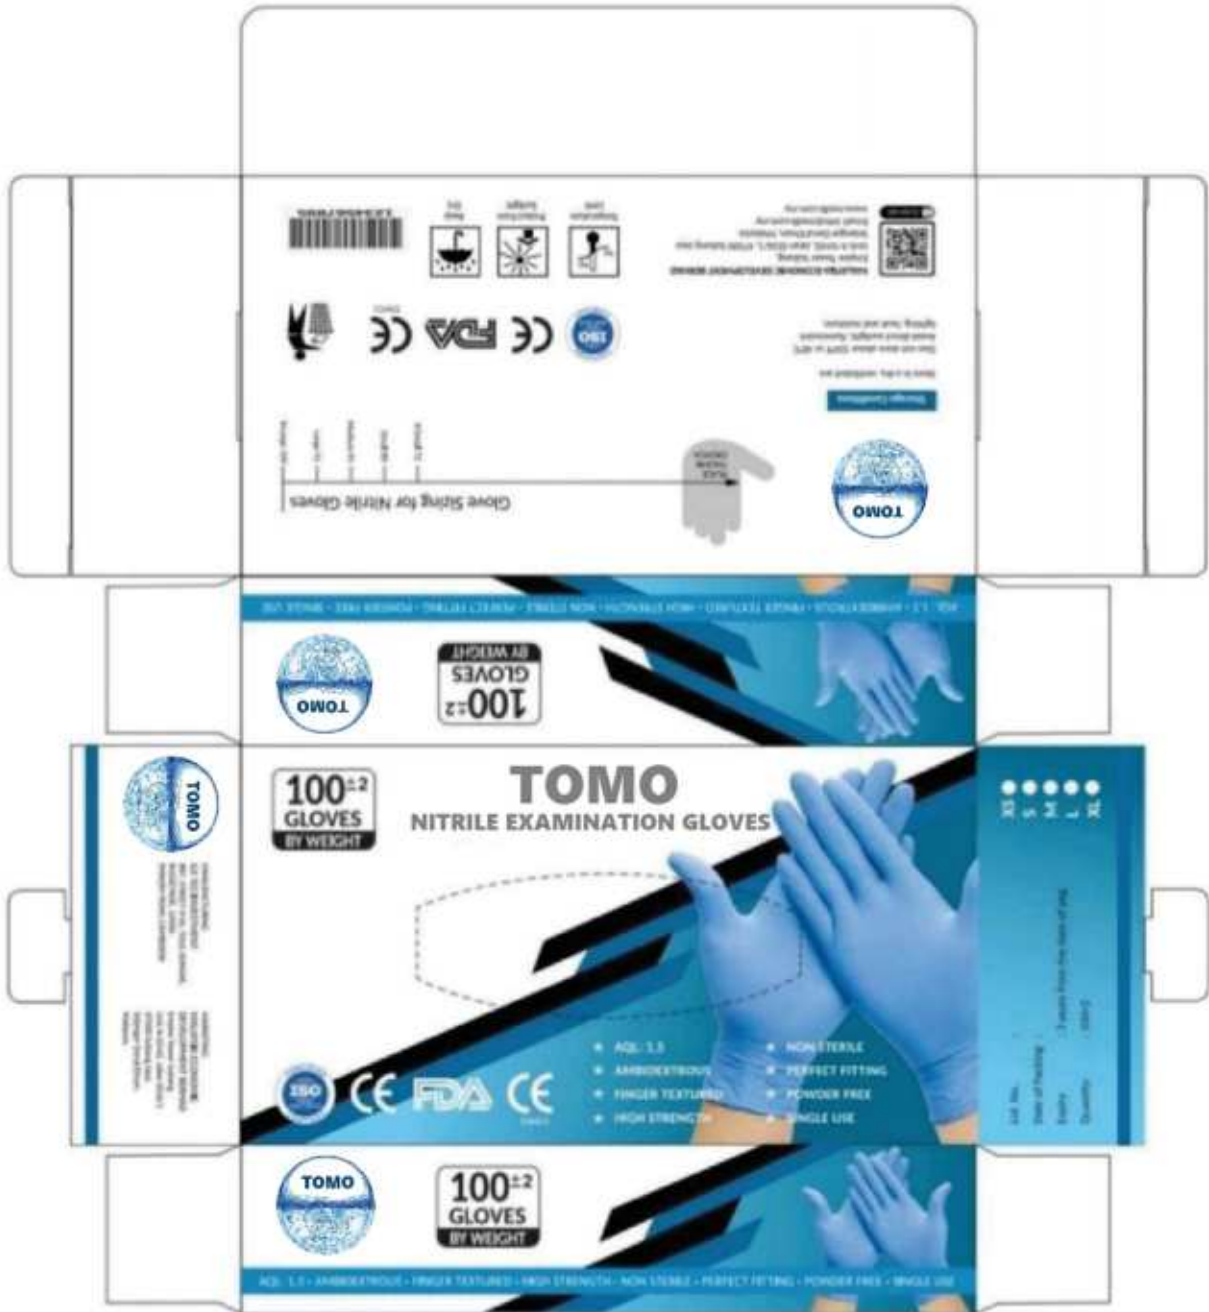



1 Box = 100pcs. / 627.2g

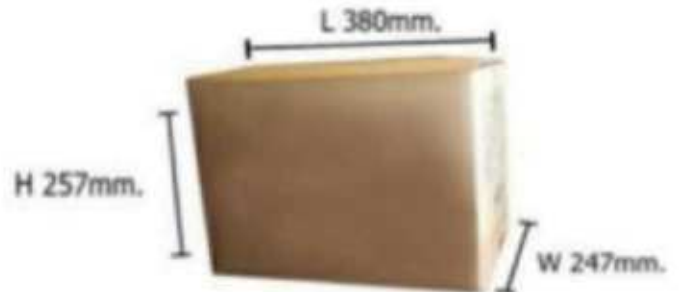

Size M : 6.27 Kg/Carton

Size L : 7.34 Kg/Carton

Approximate Weight

****1 carton = 10 boxes. = 1,000 pcs. = 0.03 CBM**

Container Dimensions



Load Container

1,200 Cartons / 20'ft

2,400 Cartons / 40'ft

2,720 Cartons / 40'HC





Certificate of Registration

This is to certify that

UNITAS CERTIFICATION SERVICES CO. LTD.

REGISTERED ADDRESS:-
PHNOM PENH, CAMBODIA.

Has been assessed and found in as per ISO 9001:2015 registration to the Requirement of standard details below.

ISO 9001:2015 (QUALITY MANAGEMENT SYSTEM)

For The Following Scope Of Activities :-

MANUFACTURERS OF POWDER FREE NITRILE GLOVE, LATEX GLOVES, 3PLY SURGICAL & MEDICAL MASK, N95, KN95, PPE KIT.

This certificate is property of Unitas Certification Services & remains valid subject to Satisfactory surveillance Audit.

Certificate No:- 1283969
Surveillance Date: - (09-SEP-2021)

Registration Date:- (09-OCT-2020)
Certificate Expiry:- (08-OCT-2023)



Chairman
Unitas Certification Services



The certificate is valid as long the organization's meet unitas certification services's requirements.
The status of the certificate may be checked at www.unitascertificationservices.co.uk

UNITAS CERTIFICATION SERVICES

Head Office : 54 Ennerdale Close, Lake, Estate, Bletchley, Milton Keynes, Buckinghamshir, Mk2 3DQ-UK
website : www.unitascertificationservices.co.uk / email: info@unitascertificationservices.co.uk



Certificate of Registration

This is to certify that

CO. LTD.

REGISTERED ADDRESS:-
PHNOM PENH, CAMBODIA.

Has been assessed and found in as per ISO 13485:2016 registration to the Requirement of standard details below.

ISO 13485:2016

(MEDICAL DEVICE-QUALITY MANAGEMENT SYSTEM)

For The Following Scope Of Activities :-

MANUFACTURERS OF POWDER FREE NITRILE GLOVE, LATEX GLOVES, 3PLY SURGICAL & MEDICAL MASK, N95, KN95, PPE KIT.

This certificate is property of Unitas Certification Services & remains valid subject to Satisfactory surveillance Audit.

Certificate No:- 139565
Surveillance Date: - (09-SEP-2021)

Registration Date:- (09-OCT-2020)
Certificate Expiry:- (08-OCT-2023)




Chairman
Unitas Certification Services



The certificate is valid as long the organization's meet unitas certification services's requirements.
The status of the certificate may be checked at www.unitascertificationservices.co.uk

UNITAS CERTIFICATION SERVICES

Head Office : 54 Ennerdale Close, Lake, Estate, Bletchley, Milton Keynes, Buckinghamshir, Mk2 3DQ-UK
website : www.unitascertificationservices.co.uk / email: info@unitascertificationservices.co.uk



Certificate of Registration

Hereby Declare That the Technical File of Product Complied with the Requirement of the (PPE 89/686/EEC)

CO. LTD.

REGISTERED ADDRESS:-
PHNOM PENH, CAMBODIA.

Has been assessed and found in as per CE MARKING registration to the requirement of standard details below.

For The Following Scope Of Activities :-
POWDER FREE NITRILE GLOVE, LATEX GLOVES, 3PLY SURGICAL & MEDICAL MASK, N95, KN95, PPE KIT.

APPLICABLE DIRECTIVE:- PERSONAL PROTECTIVE EQUIPMENT 86/686/EEC & 89/686/EEC

The Certification body has performed an audit of the above product quality system covering the design, manufacture and final inspection of the certified product. The quality system has been assessed, approved and is subject to continuous surveillance according to the

This certificate is issued under the following conditions:

1. It applies only to the quality system maintained in the manufacture of above Referenced models and it does not substitute the design or type-examination Procedures, if requested.
2. The certificate remains valid until the manufacturing conditions or the quality Systems are changed.
3. The certificate validity is conditioned by positive results or surveillance audits EC. The EC as Shown above can be used, under the responsibility of the Manufacturer, after Completion of an EC Declaration of conformity and Compliance with all relevant.
4. The statement is based on a single evaluation of one sample of above Mentioned product. It does not imply an assessment of the whole production.

This certificate is property of Unitas Certification Services & remains valid subject to Satisfactory surveillance Audit.

Certificate No:- 94521
Surveillance Date: - (09-SEP-2021)

Registration Date:- (09-OCT-2020)
Certificate Expiry:- (08-OCT-2023)



Josephine Harris

Chairman
Unitas Certification Services



The certificate is valid as long the organization's meet unitas certification services's requirements.
The status of the certificate may be checked at www.unitascertificationservices.co.uk

UNITAS CERTIFICATION SERVICES

Head Office : 54 Ennerdale Close, Lake, Estate, Bletchley, Milton Keynes, Buckinghamshir, Mk2 3DQ-UK
website : www.unitascertificationservices.co.uk / email: info@unitascertificationservices.co.uk



Certificate of Registration

Hereby Declare That the Technical File of Product Complied with the Requirement of the FDA

_____ CO. LTD.

REGISTERED ADDRESS:-
PHNOM PENH, CAMBODIA.

Has been assessed and found in as per FDA registration to the requirement of standard details below.

For The Following Scope Of Activities :-
MANUFACTURERS OF POWDER FREE NITRILE GLOVE, LATEX GLOVES, 3PLY SURGICAL & MEDICAL MASK, N95, KN95, PPE KIT.

The Certification body has performed an audit of the above product quality system covering the design, manufacture and final inspection of the certified product. The quality system has been assessed, approved and is subject to continuous surveillance according to the FDA

This certificate is issued under the following conditions:

1. It applies only to the quality system maintained in the manufacture of above Referenced models and it does not substitute the design or type-examination Procedures, if requested.
2. The certificate remains valid until the manufacturing conditions or the quality Systems are changed.
3. The certificate validity is conditioned by positive results or surveillance audits . The FDA as Shown above can be used, under the responsibility of the Manufacturer, after Completion of an FDA Declaration of conformity and Compliance with all relevant FDA.
4. The statement is based on a single evaluation of one sample of above Mentioned product. It does not imply an assessment of the whole production.

This certificate is property of Unitas Certification Services & remains valid subject to Satisfactory surveillance Audit.

Certificate No:- 199235
Surveillance Date: - (09-SEP-2021)

Registration Date:- (09-OCT-2020)
Certificate Expiry:- (08-OCT-2023)



James Hare

Chairman
Unitas Certification Services



The certificate is valid as long the organization's meet unitas certification services's requirements.
The status of the certificate may be checked at www.unitascertificationservices.co.uk

UNITAS CERTIFICATION SERVICES

Head Office : 54 Ennerdale Close, Lake, Estate, Bletchley, Milton Keynes, Buckinghamshir, Mk2 3DQ-UK
website : www.unitascertificationservices.co.uk / email: info@unitascertificationservices.co.uk